MAYO CLINIC LABORATORIES

Newborn Screen Follow-up for Elevated C0; Elevated C0/(C16+C18)

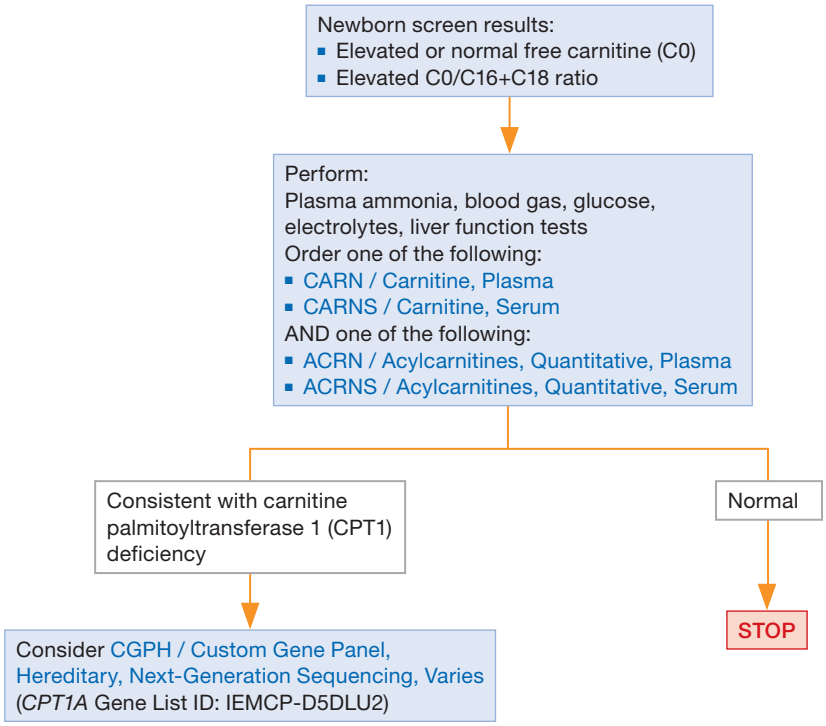

© Mayo Foundation for Medical Education and Research (MFMER). All rights reserved.