MAYO CLINIC LABORATORIES

Newborn Screen Follow-up for Elevated C16-OH +/- C18-OH

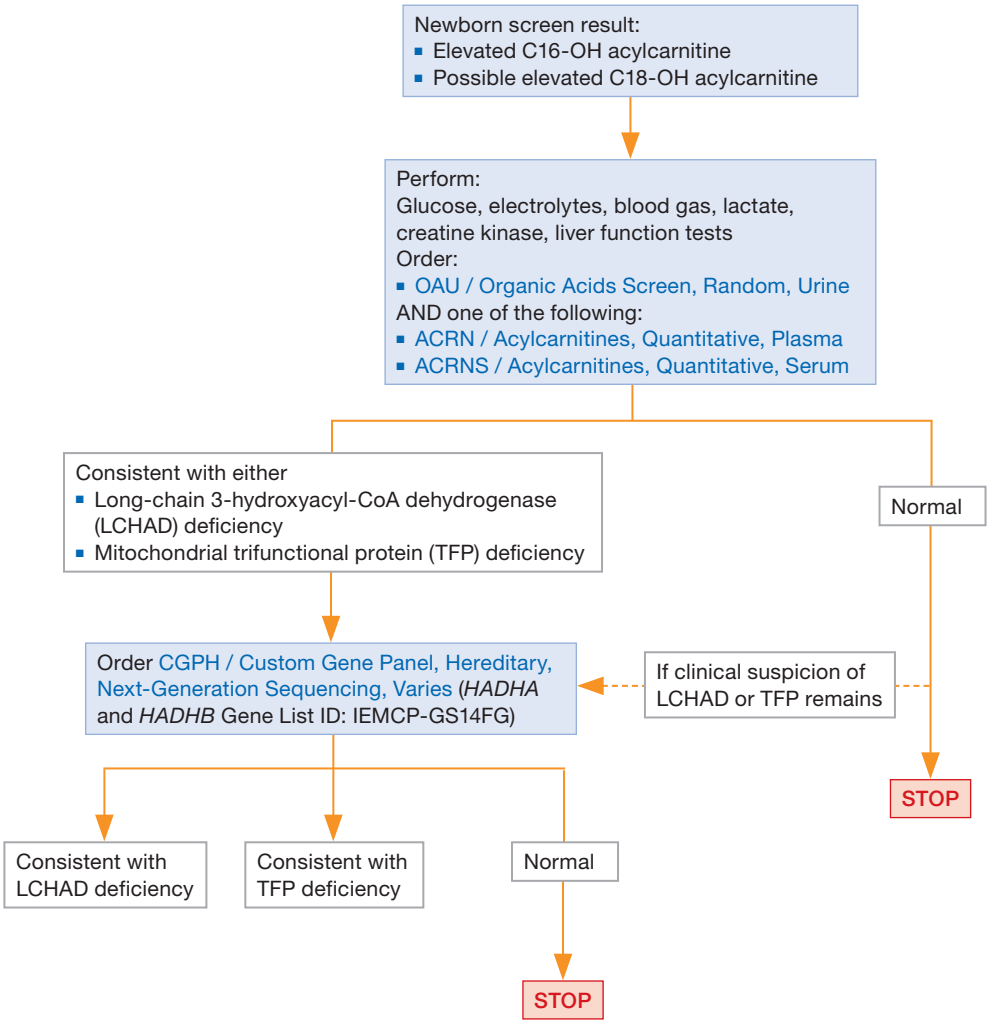

© Mayo Foundation for Medical Education and Research (MFMER). All rights reserved.