MAYO CLINIC LABORATORIES

Newborn Screen Follow-up for Elevated C8 Acylcarnitine with Lesser Elevations of C6 and C10 Acylcarnitines

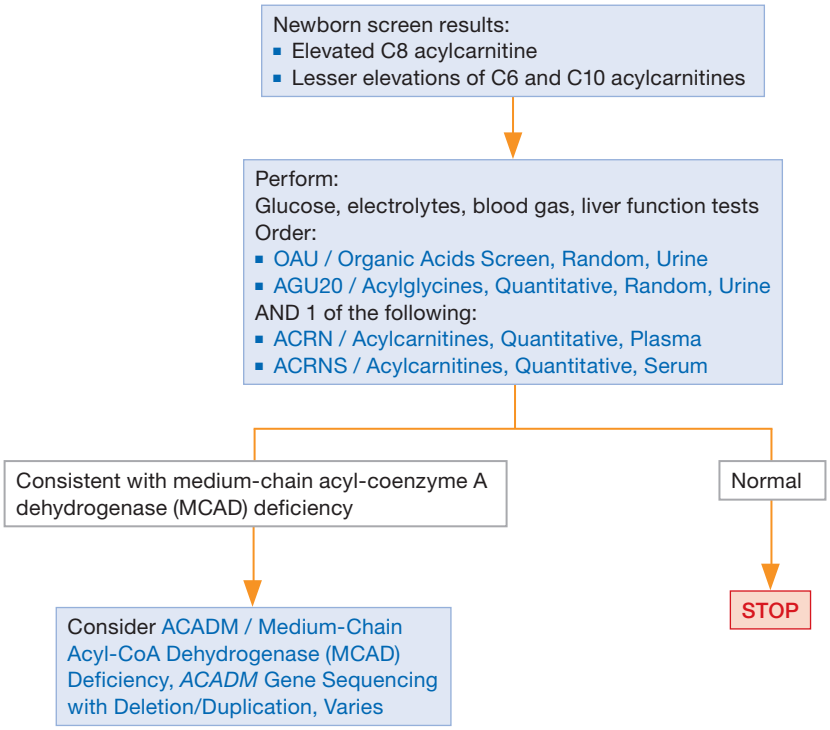

© Mayo Foundation for Medical Education and Research (MFMER). All rights reserved.