MAYO CLINIC LABORATORIES

Newborn Screen Follow-up for Elevated C16 +/- C18:1 Acylcarnitines

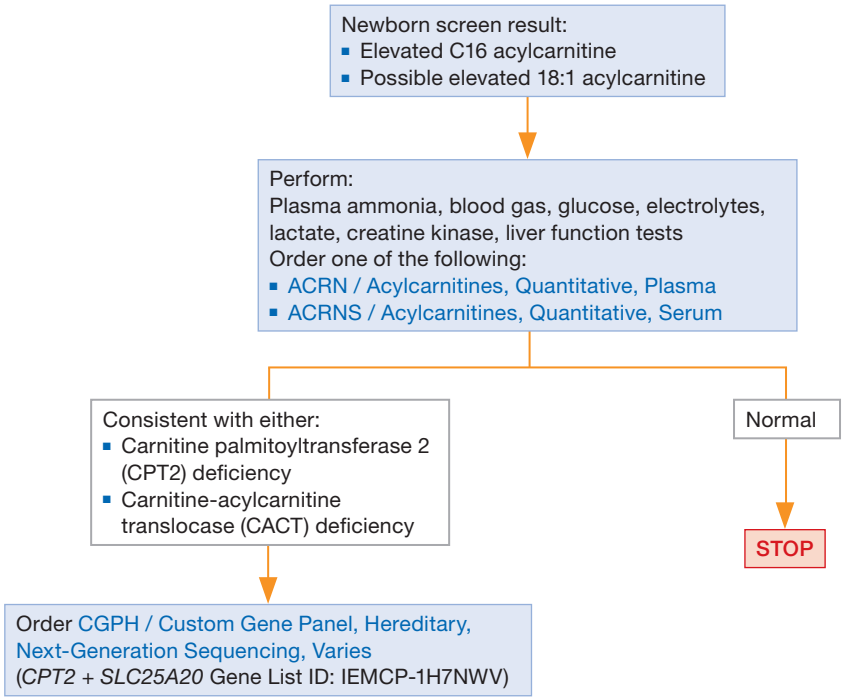

© Mayo Foundation for Medical Education and Research (MFMER). All rights reserved.